

Alarm Status

Lower	✘	Fail
Upper	✔	OK

Recorder Info

Serial #: D80202881490	Model: TRIX-8	Battery: OK	Trip #: 3	Description:
------------------------	---------------	-------------	-----------	--------------

Recorder Configuration

Start type : Push button start	Temperature alarms
Start delay : None	Lower : -4.0 °F
Interval : 5 Minutes	Upper : 158.0 °F
Alert indicator : Enabled lower & upper	
OK indicator : Enabled	

Recorded Data


First reading : 5/29/2026 9:45:54 AM	Temperature statistics
Last reading : 6/9/2026 11:35:54 AM	Lowest : -14.2 °F
Elapsed time : 11 Days 1 Hour 55 Minutes	@ 6/1/2026 9:00:54 AM
Total readings : 3191	Highest : 78.9 °F
First evaluated : 5/29/2026 9:45:54 AM	@ 5/29/2026 9:45:54 AM
Last evaluated : 6/9/2026 11:35:54 AM	Average reading: -10.9 °F
Evaluated Time : 11 Days 1 Hour 55 Minutes	Standard Deviation: 2.4 °F(S)
Evaluated Readings : 3191	MKT(ΔH 83.144): -8.2 °F

Lower Alarm

Triggered: 5/29/2026 10:05:54 AM
Time below/equal: 11 Days 1 Hour 30 Minutes
Occurrences : 1
°F - Minutes below : 111,695.00

Upper Alarm

Triggered: (none)
Time above/equal: (none)
Occurrences : 0
°F - Minutes above : 0.00

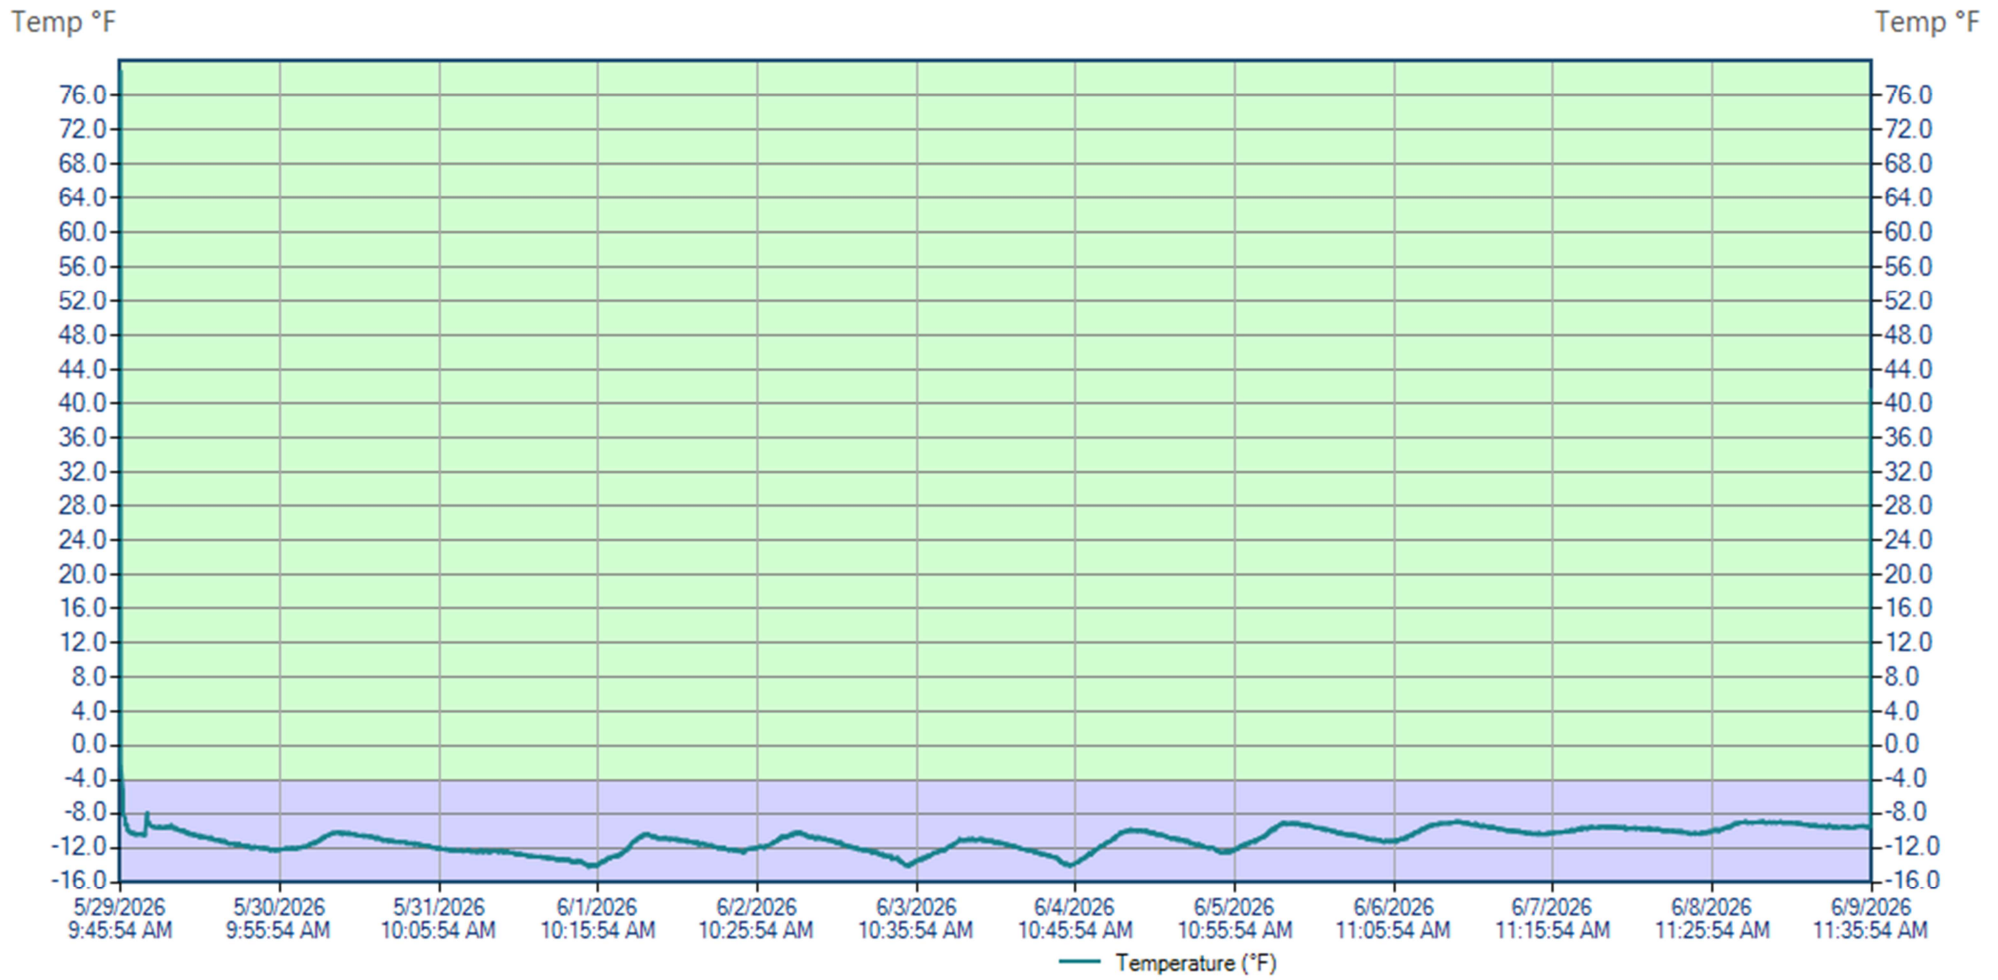

Source: TRIX-8- D80202881490 Started 5_29_2026, Finished 6_9_2026.ltd

File Location: U:\My LogTag Data

Created : 6/9/2026 11:38:28 AM