

Alarm Status

Lower	✓	OK
Upper	✓	OK

Recorder Info

Serial #: D802028822YH	Model: TRIX-8	Battery: OK	Trip #: 8	Description:
------------------------	---------------	-------------	-----------	--------------

Recorder Configuration

Start type : Push button start	Temperature alarms
Start delay : None	Lower : -4.0 °F
Interval : 5 Minutes	Upper : 158.0 °F
Alert indicator : Enabled lower & upper	
OK indicator : Enabled	

Recorded Data


First reading : 6/17/2026 12:56:33 PM	Temperature statistics
Last reading : 6/18/2026 10:46:33 AM	Lowest : 32.5 °F
Elapsed time : 21 Hours 55 Minutes	@ 6/17/2026 4:41:33 PM
Total readings : 263	Highest : 78.7 °F
First evaluated : 6/17/2026 12:56:33 PM	@ 6/17/2026 12:56:33 PM
Last evaluated : 6/18/2026 10:46:33 AM	Average reading: 37.3 °F
Evaluated Time : 21 Hours 55 Minutes	Standard Deviation: 3.9 °F(S)
Evaluated Readings : 263	MKT(Δ H 83.144): 38.2 °F

Lower Alarm

Triggered: (none)
Time below/equal: (none)
Occurrences : 0
°F - Minutes below : 0.00

Upper Alarm

Triggered: (none)
Time above/equal: (none)
Occurrences : 0
°F - Minutes above : 0.00

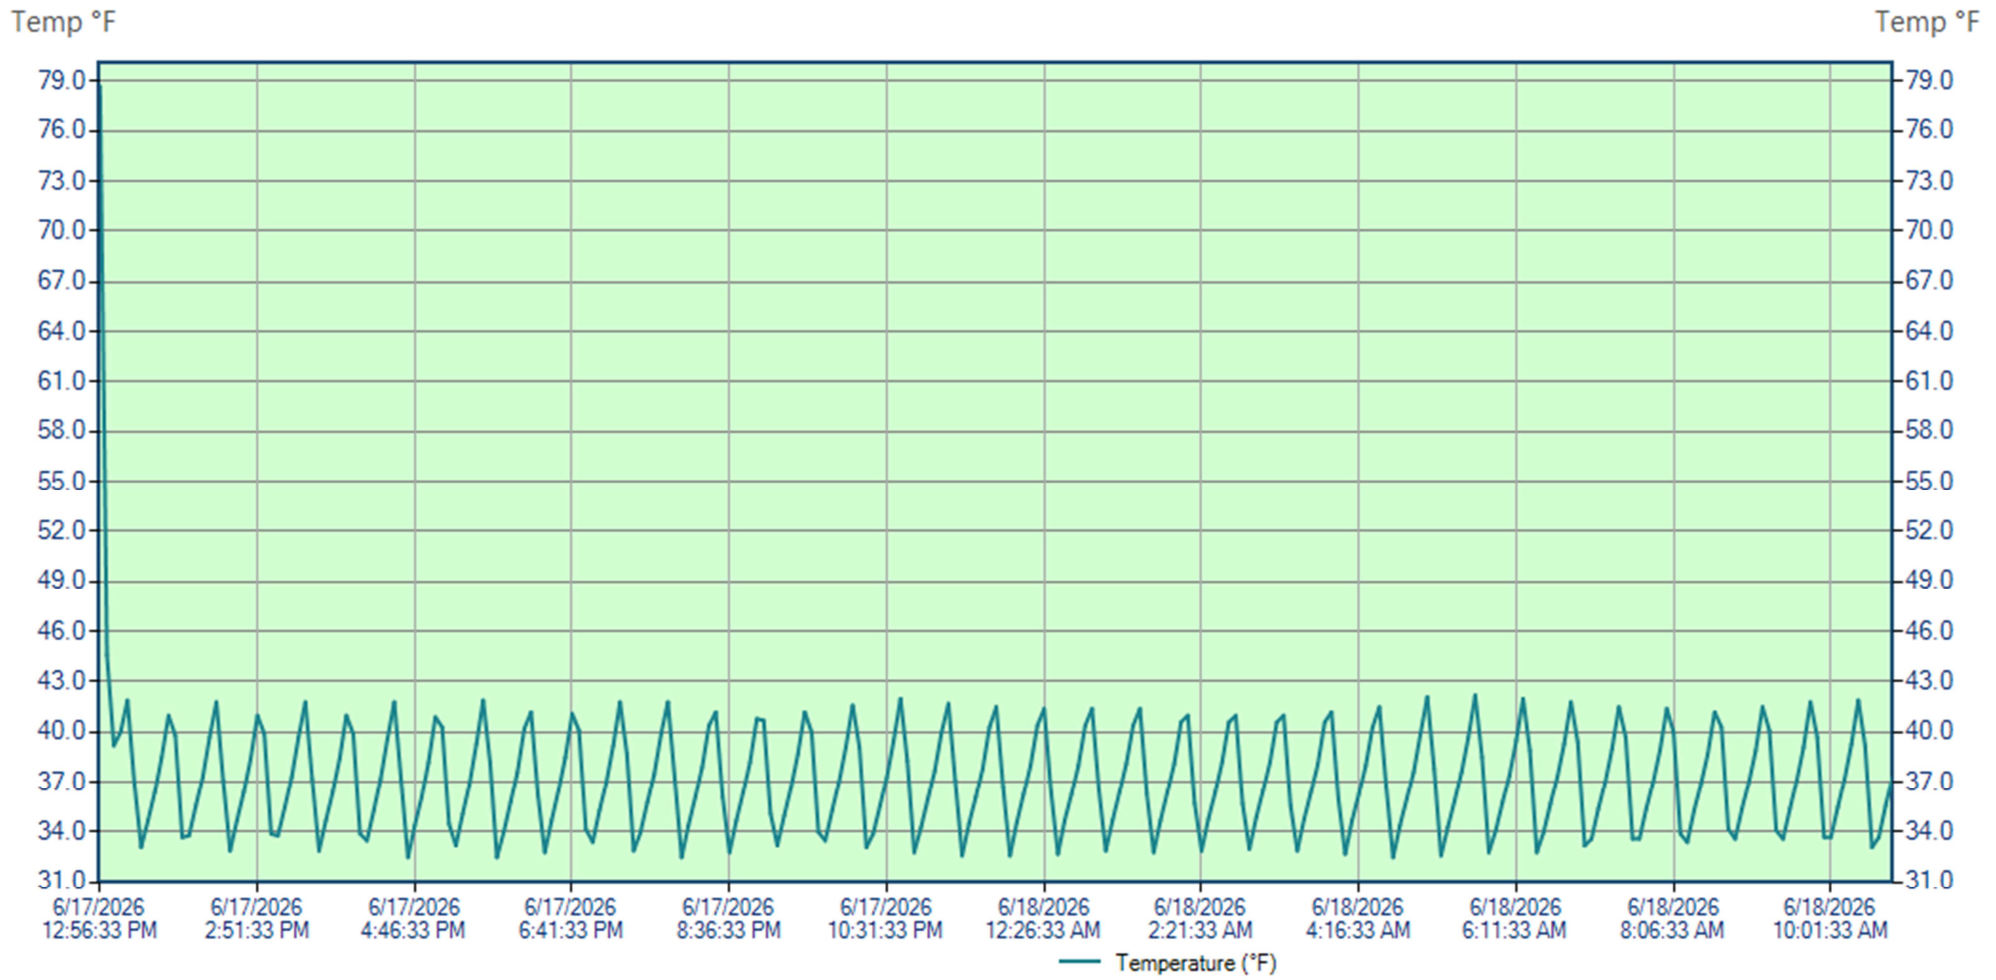

Source: TRIX-8- D802028822YH Started 6_17_2026, Finished 6_18_2026.ltd

File Location: U:\My LogTag Data

Created : 6/18/2026 10:51:08 AM